

## GEMINI SL Total Knee Replacement

**e-dur** Vit-E-Plateau

Description

As far back as the 1960s, studies confirmed that UHMWPE is an outstanding material for tribological bearing in joint replacements<sup>1,2,3</sup>.

The key properties of UHMWPE are:



- Biocompatibility
- High abrasion resistance<sup>3,4</sup>
- Impact resistance
- Fatigue strength and crack resistance

It therefore conforms to national and international standards for implant materials<sup>2,4</sup>.


Consequently, UHMWPE became the "**gold standard**" for tibial articular surfaces in knee joint reconstructions<sup>2,5</sup>. This status is confirmed by outstanding

long-term results of published studies and registry data<sup>6,7,8</sup>. Now this "**gold standard**" for orthopedic implants has been improved by further increasing its mechanical properties and durability<sup>18</sup>. Highly crosslinking produced a marked improvement in abrasion resistance<sup>9,10,11,12,13,14</sup>. In addition, effective oxidation protection is achieved by enriching the material with vitamin E<sup>9,10</sup>.

In the production of **e-dur Vit-E plateaus**, vitamin E is used as an antioxidant in order to protect the material by neutralizing the free radicals created by highly crosslinking. The product's mechanical properties and biocompatibility are preserved<sup>4,9,15,16,17</sup>.

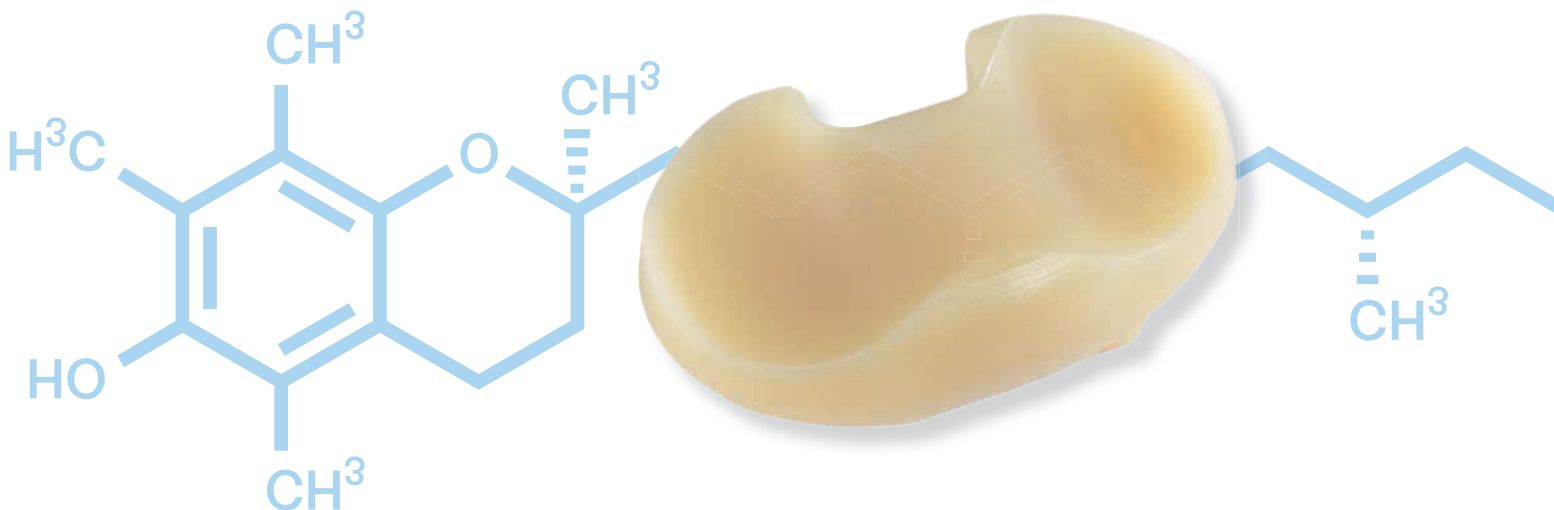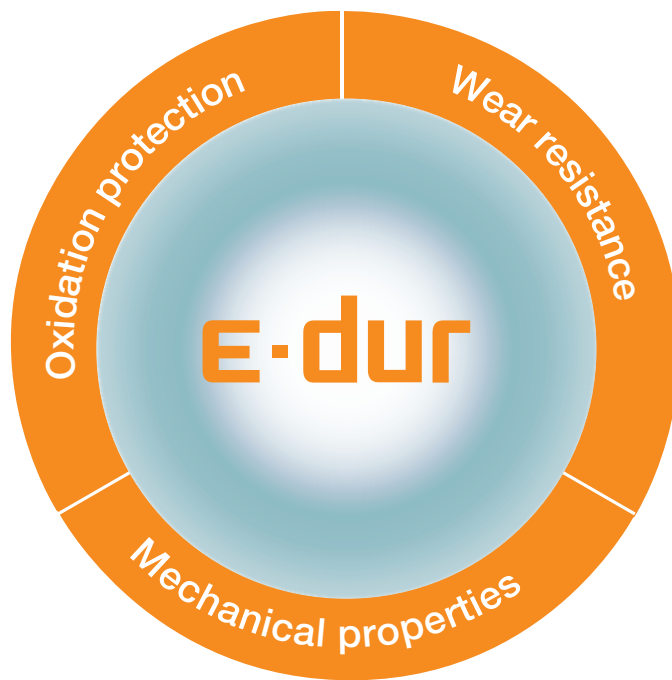


Properties

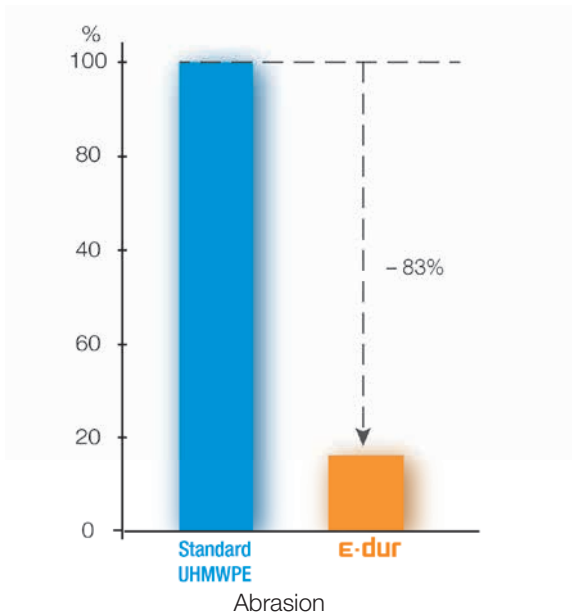

**Wear resistance**

The process of highly crosslinking produces an improvement in the abrasion resistance of UHMWPE, while enrichment with vitamin E counteracts the aging process<sup>18</sup>.

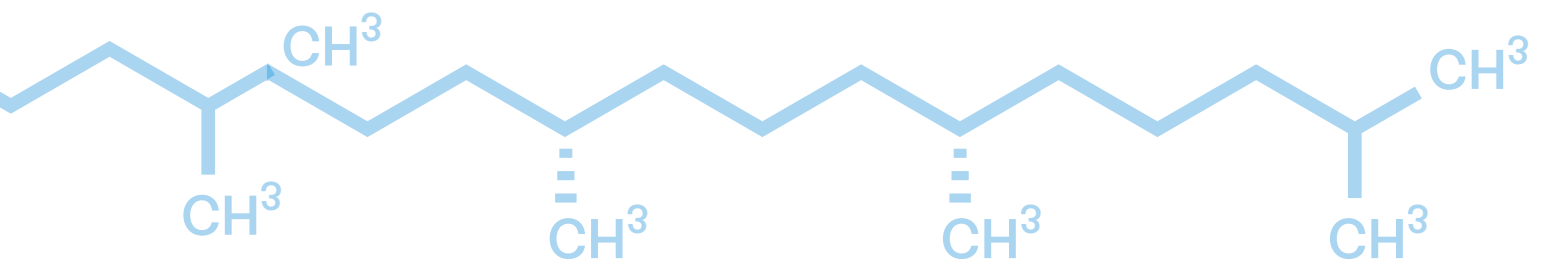

## GEMINI SL Total Knee Replacement

**Natural joint reconstruction** with physiological range of motion and functionality:<sup>19,20</sup>

- Raised femur shield
- Deep patellar articulating groove
- Physiological patella movement
- Anatomic tibia

High congruent articulation ensures uniform load transmission and high stability over the entire movement cycle.<sup>21,22</sup>



**Excellent treatment options** for a wide range of indications plus greater intraoperative flexibility:

- Modular, anatomically designed prosthesis components.
- Wide choice of sizes for every stature, irrespective of gender or ethnicity.
- Precise instrument set permits accurate axial alignment and soft tissue adjustment with optional extramedullary femoral referencing.



### Mobile Bearing


with concave tibial plateau surface

- Congruence of the articular surfaces in extension.
- Articulating femoral condyle as flexion increases, giving greater freedom of flexion and relieving strain on the patella.
- High congruence stabilizes the joint, also in the absence of the posterior cruciate ligament.

Implants

**GEMINI SL e-dur Plateaus – Mobile Bearing**


**MAT** X-LINKed Vit-E UHMWPE

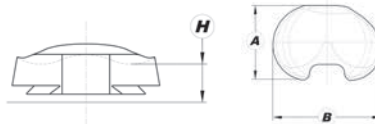


REF	Size	Side	H mm	A mm	B mm	Identification
318-801/12	x-small	right	12	42	62	R1
318-808/12	x-small plus	right	12	46	69	R1B
318-802/12	small	right	12	46	69	R2
318-807/12	medium small/medium small plus	right	12	47	74	R2A/R2B
318-803/12	medium	right	12	47	74	R3
318-804/12	large	right	12	53	78	R4
318-805/12	x-large	right	12	56	85	R5
318-811/12	x-small	left	12	42	62	L1
318-818/12	x-small plus	left	12	46	69	L1B
318-812/12	small	left	12	46	69	L2
318-817/12	medium small/medium small plus	left	12	47	74	L2A/L2B
318-813/12	medium	left	12	47	74	L3
318-814/12	large	left	12	53	78	L4
318-815/12	x-large	left	12	56	85	L5
318-801/14	x-small	right	14	42	62	R1
318-808/14	x-small plus	right	14	46	69	R1B
318-802/14	small	right	14	46	69	R2
318-807/14	medium small/medium small plus	right	14	47	74	R2A/R2B
318-803/14	medium	right	14	47	74	R3
318-804/14	large	right	14	53	78	R4
318-805/14	x-large	right	14	56	85	R5
318-811/14	x-small	left	14	42	62	L1
318-818/14	x-small plus	left	14	46	69	L1B
318-812/14	small	left	14	46	69	L2
318-817/14	medium small/medium small plus	left	14	47	74	L2A/L2B
318-813/14	medium	left	14	47	74	L3
318-814/14	large	left	14	53	78	L4
318-815/14	x-large	left	14	56	85	L5
318-801/16*	x-small	right	16	42	62	R1
318-808/16*	x-small plus	right	16	46	69	R1B
318-802/16*	small	right	16	46	69	R2
318-807/16*	medium small/medium small plus	right	16	47	74	R2A/R2B
318-803/16*	medium	right	16	47	74	R3
318-804/16*	large	right	16	53	78	R4
318-805/16*	x-large	right	16	56	85	R5
318-811/16*	x-small	left	16	42	62	L1
318-818/16*	x-small plus	left	16	46	69	L1B
318-812/16*	small	left	16	46	69	L2
318-817/16*	medium small/medium small plus	left	16	47	74	L2A/L2B
318-813/16*	medium	left	16	47	74	L3
318-814/16*	large	left	16	53	78	L4
318-815/16*	x-large	left	16	56	85	L5
318-801/18*	x-small	right	18	42	62	R1
318-808/18*	x-small plus	right	18	46	69	R1B
318-802/18*	small	right	18	46	69	R2
318-807/18*	medium small/medium small plus	right	18	47	74	R2A/R2B
318-803/18*	medium	right	18	47	74	R3
318-804/18*	large	right	18	53	78	R4
318-805/18*	x-large	right	18	56	85	R5
318-811/18*	x-small	left	18	42	62	L1
318-818/18*	x-small plus	left	18	46	69	L1B
318-812/18*	small	left	18	46	69	L2
318-817/18*	medium small/medium small plus	left	18	47	74	L2A/L2B
318-813/18*	medium	left	18	47	74	L3
318-814/18*	large	left	18	53	78	L4
318-815/18*	x-large	left	18	56	85	L5

\* The grey marked items are only available on request.

Literature, Further Information

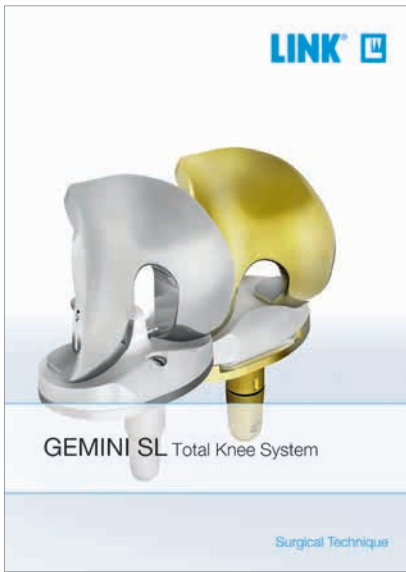





**GEMINI SL Total Knee Replacement**  
Surgical Technique

 For more information please register for our LINK Media Library ([linkorthopaedics.com](http://linkorthopaedics.com))

**Literaturquellen:**

- 1 S. M. Kurtz, „The Origins and Adaptations of UHMWPE for Knee Replacement“, in UHMWPE Biomaterials Handbook, S. M. Kurtz, Ed., Burlington, MA Academic Press 2009.
- 2 S. M. Kurtz, „Advances in the Processing, Sterilization, and Crosslinking of Ultra-high Molecular Weight Polyethylene for Total Joint Arthroplasty“, Biomaterials 1999; 20:1659-1687.
- 3 E. M. Brach del Prever, „UHMWPE for Arthroplasty: Past or Future?“, J Orthopaed Traumatol 2009; 10:1-8
- 4 Produktakte W. LINK (Quadrant, MediTECH Data Sheet)
- 5 S. M. Kurtz, „The Clinical Performance of UHMWPE in Knee Replacement“, in UHMWPE Biomaterials Handbook, S. M. Kurtz, Ed., Burlington, MA Academic Press 2009.
- 6 M. C. Forster, „Survival Analysis of Primary Cemented Total Knee Arthroplasty“, J Arthroplasty 2003; 18:265-270.
- 7 Swedish Knee Arthroplasty Register, Annual Report 2015, [www.myknee.se](http://www.myknee.se)
- 8 National Joint Registry for England, Wales, Northern Ireland and the Isle of Man, Annual Report 2015, [www.njrreports.org.uk](http://www.njrreports.org.uk)
- 9 E. Oral, „Characterization of Irradiated Blends of Alpha-tocopherol and UHMWPE“, Biomaterials 2005; 26(33):6657-6663.
- 10 E. Oral, „Alpha-tocopherol-doped Irradiated UHMWPE for High Fatigue Resistance and Low Wear“, Biomaterials 2004; 25:5515-5522
- 11 O. K. Muratoglu, „Knee Simulator Testing of Conventional and Cross-Linked Polyethylene Tibial Inserts“, J Arthroplasty 2004; 19:887-897.
- 12 O. K. Muratoglu, „Aggressive Wear Testing of a Cross-Linked Polyethylene in Total Knee Arthroplasty“, Clin Orthop Relat Res. 2002; 404:89-95.
- 13 J. T. Hodrick, „Highly Crosslinked Polyethylene is Safe for Use in Total Knee Arthroplasty“, Clin Orthop Relat Res. 2008; 466:2806-2812.
- 14 R. N. De Steiger, „Lower Prosthesis-specific 10-year Revision Rate with Crosslinked than with Non-crosslinked Polyethylene in Primary Total Knee Arthroplasty“, Acta Orthopædica 2015; 86 (6):721-727.
- 15 E. Oral, „Highly Crosslinked UHMWPE Doped with Vitamin E“, in UHMWPE Biomaterials Handbook, S. M. Kurtz, Ed., Burlington, MA Academic Press 2009.
- 16 S. M. Kurtz, „Vitamin-E-Blended UHMWPE Biomaterials“, in UHMWPE Biomaterials Handbook, S. M. Kurtz, Ed., Burlington, MA Academic Press 2009.
- 17 S. M. Kurtz, „Trace Concentration of Vitamin E Protect Radiation Crosslinked UHMWPE from Oxidative Degradation“, J Biomed Mater Res A 2008; 549-563
- 18 Testergebnis durch externes Prüflabor – Produktakte W.LINK
- 19 H. Thabe, „Auswirkungen verschiedener konstruktiver Prothesenmerkmale auf Langzeitergebnisse“, Akt Rheumatol 2013; 38
- 20 Interne Daten - H. Thabe, „Aspekte zum Konzept der beweglichen Tibiaplateaukonstruktion, April 2000
- 21 Interne Daten - A.S. Greenwald Orthopaedic Research Laboratories Report „Classification of Mobile Bearing Knee Design: Mobility and Constraint“, 2001/2002
- 22 J. Insall, „Historical Development, Classification, and Characteristics of Knee Prostheses“, in Surgery of the Knee 2nd Edition, John N., Insall Ed.; Churchill Livingstone, 1993

**CE 0482**

Explanation of Pictograms			
	Manufacturer		Article number
	Material (number)		Product meets the applicable requirements, which are regulated in the EU harmonization legislation for the affixing of the CE marking.

## Important Information

**Please note the following regarding the use of our implants:**

**1. Choosing the right implant is very important.**

The size and shape of the human bone determines the size and shape of the implant and also limits the load capacity. Implants are not designed to withstand unlimited physical stress. Demands should not exceed normal functional loads.

**2. Correct handling of the implant is very important.**

Under no circumstances should the shape of a finished implant be altered, as this shortens its life span. Our implants must not be combined with implants from other manufacturers. The instruments indicated in the Surgical Technique must be used to ensure safe implantation of the components.

**3. Implants must not be reused.**

Implants are supplied sterile and are intended for single use only. Used implants must not be used again.

**4. After-treatment is also very important.**

The patient must be informed of the limitations of the implant. The load capacity of an implant cannot compare with that of healthy bone!

**5. Unless otherwise indicated, implants are supplied in sterile packaging.**

Note the following conditions for storage of packaged implants:

- Avoid extreme or sudden changes in temperature.
- Sterile implants in their original, intact protective packaging may be stored in permanent buildings up until the "Use by" date indicated on the packaging.
- They must not be exposed to frost, dampness or direct sunlight, or mechanical damage.
- Implants may be stored in their original packaging for up to 5 years after the date of manufacture. The "Use by" date is indicated on the product label.
- Do not use an implant if the packaging is damaged.

**6. Traceability is important.**

Please use the documentation stickers provided to ensure traceability.

**7. Further information** on the material composition is available on request from the manufacturer.

**Follow the instructions for use!**

### **Waldemar Link GmbH & Co. KG, Hamburg**

All content in this catalog, including text, pictures and data, is protected by law. Every instance of use, whether in part or in whole and which is not permitted by law, is subject to our prior consent. In particular, this applies to the reproduction, editing, translation, publishing, saving, processing, or passing on of content stored in databases or other electronic media and systems, in any manner or form. The information in the catalogs is solely intended to describe the products and does not constitute a guarantee.

The Surgical Technique described has been written to the best of our knowledge and belief, but it does not relieve the surgeon of his/her responsibility to duly consider the particularities of each individual case.

Products shown in this document may not be available in your country. The product availability is subject to the approval and/or registration regulations of the respective country. Please contact Waldemar Link GmbH & Co. KG if you have questions about the availability of LINK products in your country.

Waldemar Link GmbH & Co. KG and/or other corporate affiliated entities own, use or have applied for the following trademarks in many jurisdictions: LINK, BiMobile, SP II, Modell Lubinus, E-Dur, EndoDur, T.O.P. II, BetaCup, CombiCup PF, CombiCup SC, CombiCup R, MobileLink, C.F.P., LCU, SP-CL, LCP, MIT-H, Endo-Model, Endo-Model SL, MP, MEGASYSTEM-C, GEMINI SL, SPAR-K, LCK, Link OptiStem, HX, TiCaP, X-LINKed, PorAg, LINK PorEx, BiPorEx, PorEx-Z, TrabecuLink, Tilastan, customLINK, RescueSleeve, Stactip, VACUCAST.

Other trademarks and trade names may be used in this document to refer to either the entities claiming the marks and/or names or their products and are the property of their respective owners.



Waldemar Link GmbH & Co. KG

Barkhausenweg 10 · 22339 Hamburg · Germany  
Phone +49 40 53995-0 · [info@linkhh.de](mailto:info@linkhh.de)  
[www.linkorthopaedics.com](http://www.linkorthopaedics.com)

